
MRI RF Coil, LNA and Diode Section



Non-magnetic components are often specified for this section of the overall MRI system.

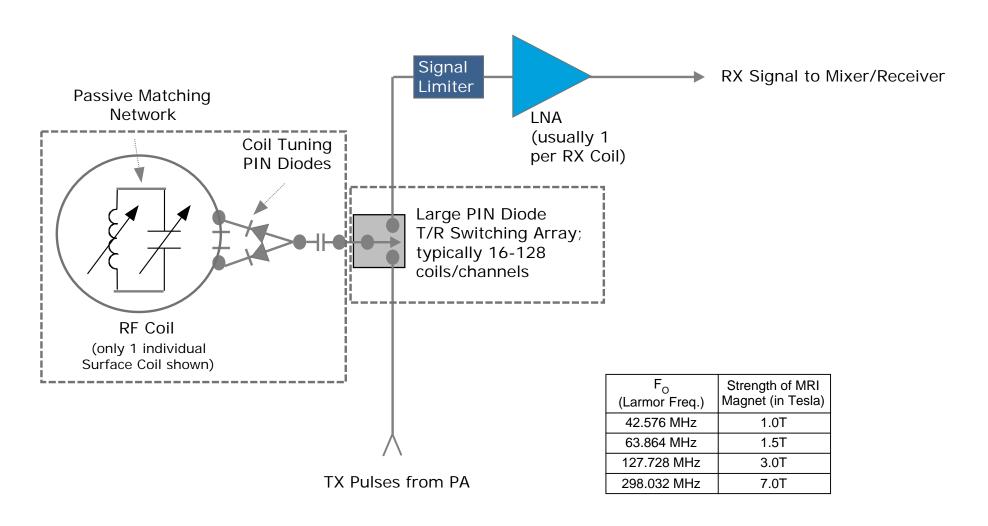